



Uric Acid

Colorimetric Microplate Assay Kit

User Manual

Catalog # CAK1058

(Version 1.4D)

Detection and Quantification of Uric Acid(UA)Content in Urine,
Serum, Plasma, Other biological fluidsSamples.

For research use only. Not for diagnostic or therapeutic procedures.

I. INTRODUCTION.....	2
II. KIT COMPONENTS.....	3
III. MATERIALS REQUIRED BUT NOT PROVIDED.....	4
IV. REAGENT PREPARATION.....	5
V. SAMPLE PREPARATION.....	6
VI. ASSAY PROCEDURE.....	7
VII. CALCULATION.....	8
VIII. TYPICAL DATA.....	9

I. INTRODUCTION

In humans and primates, uric acid is the end product of purine metabolism. It is produced by the oxidation of xanthine and hypoxanthine by xanthine oxidase and excreted in urine. High serum levels of uric acid, hyperuricemia, are associated with insulin resistance, cardiovascular disease, and gout. The mechanisms leading to hyperuricemia are typically either increased uric acid production or decreased urine excretion. Increased serum uric acid may be a marker of renal disease.

Uric Acid Colorimetric Microplate Assay Kit provides a simple and direct procedure for measuring uric acid content in a variety of samples. The assay is initiated with the enzymatic catalysis of the uric acid by uricase. The enzyme catalysed reaction products quinone can be measured at a colorimetric readout at 550 nm.

II.KIT COMPONENTS

Component	Volume	Storage
96-Well Microplate	1 plate	
Diluent	20mlx 1	4 °C
Enzyme	Powderx 1	-20 °C, keep in dark
Dye Reagent	Powder x 1	-20 °C, keep in dark
Standard (4mmol/L)	1 ml x 1	4 °C
Plate Adhesive Strips	3 Strips	
Technical Manual	1 Manual	

III. MATERIALS REQUIRED BUT NOT PROVIDED

1. Microplate reader to read absorbance at 550 nm
2. Distilled water
3. Pipettor, multi-channel pipettor
4. Pipette tips
5. Mortar
6. Centrifuge
7. Timer
8. Ice

IV. REAGENT PREPARATION

Standard: Briefly centrifuge prior to opening. Perform 2-fold serial dilutions of the top standard solution using distilled water to make the standard curve. The concentration of standard curve could be 4/2/1/0.5/0.25/0.125/0.0625 mmol/L.

Enzyme: Add 10 ml Diluent to dissolve before use. Keep in dark and store at 4 °C for 1 week after reconstitution.

Dye Reagent: Add 10 ml Diluent to dissolve before use. Keep in dark and store at 4 °C for 2-3 weeks or -20 °C for 2 months.

V. SAMPLE PREPARATION

1. For urine, serum or plasma samples

Detect directly.

VI. ASSAY PROCEDURE

Warm all reagents to room temperature before use.

Add following reagents into the microplate:

Reagent*	Standard	Blank	Sample*
Enzyme	100 μ l	100 μ l	100 μ l
Standard	10 μ l	--	--
Distilled water	--	10 μ l	--
Sample	--	--	10 μ l
Dye Reagent	100 μ l	100 μ l	100 μ l
Mix, put it in the oven, 37 °C for 15 minutes, measured at 550 nm and record the absorbance.			

Note:

*Reagents must be added sequentially and should not be premixed prior to addition.

**The concentrations can vary over a wide range depending on the different samples.

For unknown samples, we recommend doing a pilot experiment & testing several doses to ensure the readings are within the standard curve range.

**For colored samples, we recommend setting a parallel sample background control well with same volume of sample only. Other reagents were replaced by distilled water to the same total volume. Subtract the OD value of the sample background control from the OD value of the sample to correct for interference from the sample's own color.

VII. CALCULATION

1. Calculate the sample concentration in ASSAY PROCEDURE according to the slope of the standard curve

$$C = \frac{(OD_{\text{Sample}} - OD_{\text{Blank}}) - \text{Intercept}}{\text{Slope}} \times \frac{V_{\text{Standard}}}{V_{\text{Sample}}} \times n (\text{mmol/L})$$

Calculate the initial concentration according to sample preparation procedure.

2. According to one point of the standard OD and concentration

$$C = \frac{(C_{\text{Standard}} \times V_{\text{Standard}}) \times (OD_{\text{Sample}} - OD_{\text{Blank}})}{(OD_{\text{Standard}} - OD_{\text{Blank}}) \times V_{\text{Sample}}} (\mu\text{mol/ml})$$

Slope: the absorbance slope of standard curve

n: the dilution factor


C_{Standard} : the standard concentration, $\text{mmol/L} = \mu\text{mol/ml}$

V_{Standard} : the volume of standard in assay procedure, μl

V_{Sample} : the volume of sample in assay procedure, μl

VIII. TYPICAL DATA

The standard curve is for demonstration only. A standard curve must be run with each assay.

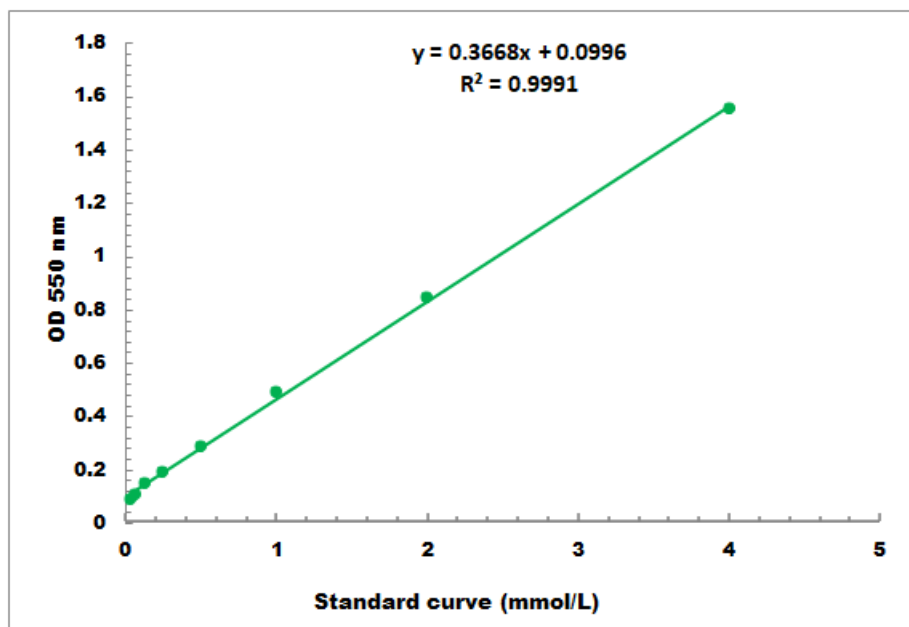

Detection Range: 0.04 mmol/L - 4 mmol/L